


# NIDEK Medical

## INSTRUCTIONS FOR USE

### Mark 5 Nuvo Family (NUVO, NUVO 8 & NUVO 10) OXYGEN CONCENTRATOR

For models: 505, 565, 585, 595, 905, 965, 985 and 1005  
(and variants thereof)

[Original language is English]

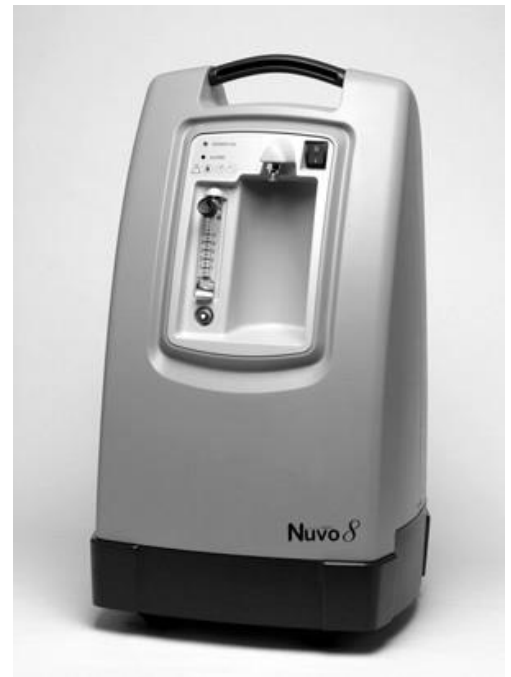
















NUVO 8 (Model 985) shown for reference.

	This unit is not a life-support device. Geriatric, pediatric, or any other patient unable to communicate discomfort while using this device should receive additional monitoring.
  	<p>This device supplies highly concentrated oxygen enriched product gas that promotes rapid burning.</p> <p>DO NOT allow smoking or open flames within the same room of this device or the administration accessory (cannula). Failure to observe this warning can result in severe fire, property damage, and / or cause physical injury or death.</p>
 	Oxygen accelerates the combustion of flammable substances. DO NOT use oil, grease, petroleum based or other flammable products on the device, the administration accessory (cannula) or the patient's face / neck.
	Only persons who have read and understood this entire manual should be allowed to operate the device.
	<b>CONTRAINDICATIONS</b> - Those who continue to smoke (because of the increased fire risk and the probability that the poorer prognosis by smoking will offset the treatment benefit).
	Federal Law (US) restricts this device to sale by, or on the order of, a licensed physician. This oxygen concentrator should be used only under the supervision of a licensed physician.

## Contents

GLOSSARY OF SYMBOLS .....	2
YOUR DEVICE.....	2
Intended Use and Operation.....	2
Device Features.....	2
Alarms and Safety Features .....	3
Device Performance and Specifications .....	3
Accessories and Spare Parts.....	4
UNPACKING AND INSPECTION .....	4
INSTALLATION AND OPERATION .....	4
Installation.....	4
Start-Up.....	5
Shut Down .....	5
CLEANING AND MAINTENANCE .....	5
Cleaning .....	5
Maintenance .....	5
DISPOSAL .....	6
Method for Waste Disposal .....	6
Disposing of the Device.....	6
TROUBLESHOOTING.....	6
EMC INFORMATION.....	7
CONFORMITY WITH EN 60601-1 .....	8

## GLOSSARY OF SYMBOLS

	ON (Power switched on)
	OFF (Power switched off)
	Manufacturer Name and Address
	Type B Device
	Class II Protection
<b>IPX1</b>	Protection from vertically falling water drops
	Do Not Expose to Open Flames
	Do Not Expose to Oil or Grease
	Tools Required / Technician Only
	Refer to Technical Information / Service Manual
	Refer to Instructions for Use / User's Guide
	Keep in Vertical Position
	FRAGILE – Handle with Care
	Oxygen Concentration Indicator Warning
	WARNING – A hazard or unsafe practice that can result in serious injury or death if conditions are not avoided.
	Caution - A hazard or unsafe practice that can result in minor injury and / or property damage if conditions are not avoided.
	Note – Information important enough to emphasize or repeat
<b>CE</b> 0413	The Nuvo Family was manufactured in a plant with a Quality Management System certified as being in conformity with ISO 13485:2003

## YOUR DEVICE


### Intended Use and Operation

The Mark 5 Nuvo Family (Nuvo, Nuvo 8 and Nuvo 10) Oxygen Concentrators are used as a means of providing continuous oxygen enriched product gas for patients, adolescent to geriatric, suffering from health conditions that cause low levels of oxygen in the blood (hypoxaemia).

The Mark 5 Nuvo Family begins their operation with air being pulled into the external air intake filter. This


filtered air enters the compressor via a suction resonator and fine filter. Pressurized air then exits the compressor and passes through a heat exchanger, which reduces the temperature of the compressed air. Next, an electronic valve system directs the air into one of two tubes that contain molecular sieve (sieve beds). The molecular sieve adsorbs (physically attracts) the nitrogen from the air as it is pushed through the sieve beds, this process is called pressure swing adsorption (PSA). This allows the oxygen enriched product gas to pass through before being delivered to the pressure regulator. As one tube is generating the product gas, the other is being purged of the adsorbed nitrogen. After passing through the regulator, the rate of product gas being delivered to the patient is set by the flow meter adjusting valve. Finally, it passes through a fine particle filter and then over a sensor that detects the oxygen concentration of the product gas before it exits the device through a fire resistant outlet.

### Device Features

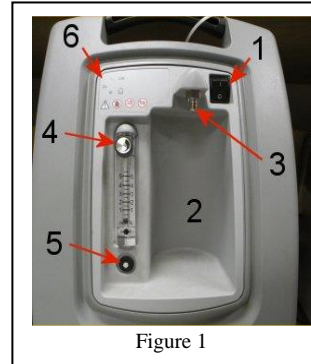


#### Front panel (Fig. 1)

- 1 - Power Switch
- 2 - Humidifier
- (space reserved)
- 3 - Oxygen product outlet
- 4 - Flow adjustment knob (LPM)
- 5 - Circuit Breaker
- 6 - Indicator Lights (red and green)

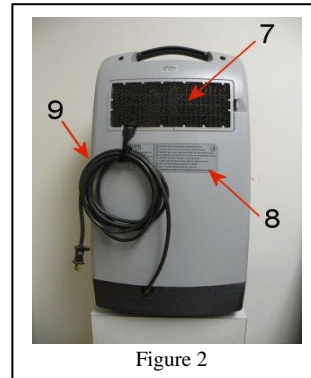



#### Rear panel (Fig. 2)

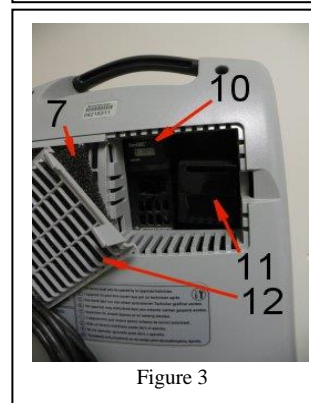- 7 - Cabinet Air Filter
- 8 - Manufacturer's Technical Label
- 9 - Mains Cable




#### Rear panel (Fig. 3)


- 10 - Hour meter
- 11 - Filter / Silencer
- 12 - Ventilation Grille

	Use the power cord provided, and check that the electrical characteristics of the power socket used match those indicated on the manufacturer's plate on the rear panel of the device.
	This unit may be equipped with a polarized plug. That is one blade wider than the other. If it does not fit into the outlet, reverse the plug. If it still does not fit, contact a qualified electrician. Do not defeat this safety feature.

### Alarms and Safety Features

	The device has an audible alarm to warn the user of problems. In order that the alarm may be heard, the maximum distance that the user can move away from it must be determined to suit the surrounding noise level.
---	--

**No voltage detection:** In the event of a loss of mains power, an intermittent audible alarm is activated and the green light turns off.

	Test alarm by actuating the Power Switch (Fig 1-1) when the power cord is not plugged into the wall receptacle.
---	---


**Oxygen Concentration Status Monitor:** The oxygen concentration monitor is an electronic module capable of checking the effective oxygen concentration supplied by the concentrator. The oxygen monitor measures the concentration and activates an audible and visual alarm if it falls below the alarm set point percentage. When the device is started, the indicator lights (Fig 2-6) located on the front panel operate as described below.

**Green indicator:** The green indicator light indicates that power is applied to the concentrator and that it is ready to provide oxygen enriched air to the patient.

To be lit, it is necessary that the concentrator power plug be inserted into the wall outlet, that the Power Switch (Fig 1-1) be actuated and that the oxygen concentration has reached the alarm set-point. On initial power up it will flash green until the unit has reached normal operating conditions (approximately 2 minutes).

**Red indicator:** This indicator will light when the oxygen concentration level falls below the set point. After 15 minutes ( $\pm 2$  minutes) of the indicator light being lit, a continuous audible alarm is activated.

If the alarm is actuated, press the Power Switch (Fig 1-1) to the "O" (OFF) position to stop the device and call the equipment supplier to service the device.

	No special maintenance is required. The alarm set-point is factory set and the setting cannot be adjusted. All OCSI models are set at $85\% \pm 3\%$ .
---	--

**No Flow detection:** If supplied, the device has a Blockage Alarm. A continuous audible alarm and both indicator lights will be lit immediately in the event the flow of oxygen to patient becomes blocked.

**Thermal safety:** The compressor motor is protected by a thermal switch situated in the stator winding ( $145 \pm 5^\circ \text{C}$ ). One tubeaxial fan cools the compressor compartment and additional fans cool the heat exchanger coil for the Nuvo 8 and Nuvo 10 models (585, 985, 595, and 1005)

### Electrical protection:

- A 5A circuit breaker is incorporated into the front cabinet of all 230V models
- A 10A circuit breaker is incorporated into the front cabinet of all 115V models
- Class II devices with insulated castings (EN60601-1 standard)



**Safety valve:** This is fitted on the compressor outlet and is calibrated to 3.4 bar (50 psig).

**Fire Break:** This device is fitted with a metal fire break at the Oxygen Product Outlet (Fig 1-3). This break will keep fire from entering the device.

### Device Performance and Specifications

The performance of the device (especially the oxygen concentration) are quoted at  $21^\circ \text{C}$  ( $70^\circ \text{F}$ ) and one atmosphere. They may change with temperature and altitude.

Model	505/565	905/965	585	985	595	1005
<b>Description</b>	5lpm 115V	5LPM 230V	8LPM 115V	8LPM 230V	10LPM 115V	10LPM 230V
<b>Frequency</b>	60Hz	50/60Hz	60Hz	50/60Hz	60Hz	50Hz
<b>Average Power</b>	410 Watts	420 Watts	500 Watts	490 Watts	700 Watts	600 Watts
<b>Protection Class</b>	Class II					
<b>Mains Protection</b>	10A	5A	10A	5A	10A	5A
<b>Average Oxygen Content</b>	At 2 LPM > 90%		At 2 LPM > 90%		At 2 LPM > 90%	
<b>Average Oxygen Content</b>	At 5 LPM 87% to 95.5%		At 8 LPM 87% to 95.5%		At 10 LPM 87% to 95.5%	
<b>Liter Flow</b>	1 to 5 LPM		2 to 8 LPM		2 to 10 LPM	
<b>Outlet Pressure</b>	7 Psig		15 Psig		20 Psig	
<b>Dimensions (L x W x H)</b>	394 x 396 x 706 mm (15.5 x 15.6 x 27.8 in.)					
<b>Weight</b>	24 kg (54 lbs)					
<b>Noise Level</b>	within ISO 8359 guidelines					

	In compliance with the ISO 8359 standard, the flow supplied is equal to the flow set on the flowmeter, accurate to within $\pm 10\%$ or 200 ml/min, whichever is the larger of the two.
	The variation of the maximum recommended flow does not exceed $\pm 10\%$ of the indicated value when a back pressure of 6.9 kPa (1 psig) is applied to the output of the device.

### Materials in direct or indirect contact with the patient

Concentrator enclosure	ABS/Polycarbonate
Printed labels	Polycarbonate
Power switch (Fig 1-1)	Nylon
Oxygen product outlet (Fig 1-3)	SS or Brass
Flow adjustment knob (Fig 1-4)	ABS



Cabinet air filter (Fig 2-7)	Polyester
Mains cable (Fig 2-9)	PVC
Filter / Silencer (Fig 3-11)	Polypropylene
Humidifier	Polypropylene
Casters	Nylon
Pipe/Tubing	Aluminum, PVC, polyurethane and/or silicone

### Accessories and Spare Parts

The accessories used with the *device* must be oxygen compatible, designed for oxygen therapy use, biocompatible and comply with the general requirements of the FDA Quality System Regulation or the 93/42/EEC European Directive, or any other applicable regulatory requirements.

The accessories below, available from **Nidek Medical Products, Inc.** and our distributors, comply with these requirements. Contact your equipment supplier to obtain these accessories.

Accessories	Part Ref
Humidifier (1 to 5 LPM)	9012-8774
High Flow Humidifier (2 to 10 LPM)	9251-8774
Cannula with 2m (7ft) tubing (1 to 5 LPM)	9012-8780
High Flow Cannula with 2m (7ft) tubing (2 to 10 LPM)	9251-8780
Extension Tubing 7.7m (25 ft)	9012-8781
Tubing Adapter	9012-8783
Adapter, DISS to hose	9012-8785

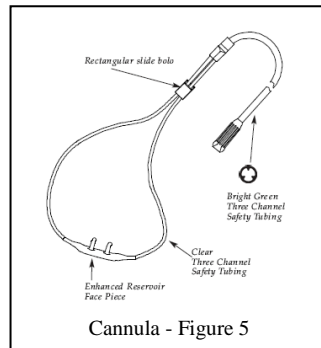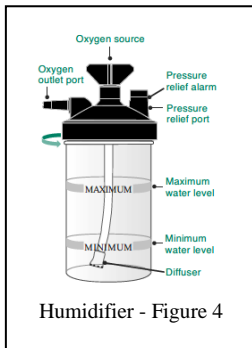

	The use of certain administration accessories which are not specified for use with this concentrator may reduce its performance and void the manufacturer's responsibility (ISO 8359).
--	--

Spare Parts	Part Ref
Cabinet air filter (Fig 2-7)	9250-1025
Filter / Silencer (Fig 3-11)	9250-1180
Ventilation Grille (Fig 3-12)	9250-1006
Casters	8300-8068
Mains Cable Wrap	8400-0022

	Please consult the Nuvo Family Service Manual (PN 2010-2329) for instructions on replacing any above spare parts.
--	---

## UNPACKING AND INSPECTION

The Oxygen Concentrator is packaged to protect the device from damage while being transported and stored. After the device is removed from the package, inspect for damage. If damage is detected, please contact your equipment provider.

If you do not plan to use your device immediately, please consult the Environmental Storage Conditions below.

### Environmental Storage Conditions:

The device should be stored in a dry area, with an ambient temperature between -20°C to 60°C (0°F to 140°F) at 15-95% relative humidity. It must be stored, transported and used in the vertical position only.

Oxygen concentration can be affected after prolonged periods of storage – check device before use.

## INSTALLATION AND OPERATION






### Installation

### Environmental Operating Conditions:

The device should be operated in a dry area, with an ambient temperature between 10°C to 40°C (50°F to 105°F) at 15-95% relative humidity. The device can be operated at an altitude of up to 1500m (5000ft) at a temperature of 21°C (70°F) without causing product degradation.

	Petroleum and oil based lubricants are flammable and the use of them with the device is not recommended.
	Improper patient connection to and use of the cannula may result in injury, including strangulation. To reduce the risk of this occurring, avoid situations that might cause the cannula or hose to become entangled about the patient's neck and do not attach more than 15.5m (50 ft) in length of tubing.
	Ears, nose and neck may become irritated after prolonged exposure to the cannula. For relief, only a water based lubricant is recommended.
	Nasal passages may become irritated after prolonged exposure to the product gas. If this occurs, consult your physician about using a humidifier during treatment.


	DO NOT use in explosive atmosphere. To avoid risk of fire and explosion the concentrator should be kept away from heat sources, incandescent sources, solvents, Aerosols, etc.
	Unit should be placed and operated in a well-ventilated space that is free of pollutants or fumes and protected from the elements with adequate lighting.
	For patient safety and benefit, no modification to the equipment is allowed. It is also not recommended to interconnect the device with any equipment or accessories not specified in this guide.

	Device must have power to operate. In the event of power loss and for continued operation a backup source is recommended.
	Do not use in a specifically magnetic environment (MRI, X-ray, etc.). May cause device malfunction.
	We recommend against the use of extension cords and adapters, as they are potential sources of sparks and fire.
	Consult your equipment provider for further information regarding altitudes of 1500 m to 4000m (5000 to 13000ft).
	Complies with EN 60601-1:2003 standard; spilling of a glass of water.

### Start-Up


- 1) Ensure that the Power Switch (Fig 1-1) is in the "●" (OFF) position.

*If used with a humidifier (Fig 4):* Unscrew the flask and fill it with distilled water up to the line (see manufacturer's instructions). Then screw the lid on the humidifier flask until there are no leaks. Connect the oxygen tube to the humidifier outlet nozzle. Screw the humidifier directly to the Oxygen Product Outlet (Fig 1-3). Ensure that all of the parts are connected correctly so as to avoid leaks.


	Replace water in humidifier bottle before each treatment.
--	---


*If not using a humidifier:* Attach a DISS to hose Adapter (PN 9012-8785) to the Oxygen Product Outlet (Fig 1-3). Connect the oxygen tube to the adapter.

- 2) Plug the power cable into a power outlet of the correct voltage and frequency as defined on the manufacturer's technical label (Fig 2-8).
- 3) Press the Power Switch (Fig 1-1) to the ON "I" position.

	See the Alarms and Safety Features on page 3 for indicator lights and meanings.
---	---

- 4) Turn the flow adjustment knob (Fig 1-4) to the prescribed value.



	View the flowmeter from straight on for accurate settings.
---	--

	The required oxygen concentration is normally obtained within two minutes after the device is started.
---	--

- 5) Check that the oxygen flows out of the administration device (nasal cannulas or other) by placing the orifice(s) on the surface of a glass of water. The flow should disturb the surface of the water.
- 6) Adjust the nasal cannula to suit your face.

### Shut Down


At the end of the treatment, press the Power Switch (Fig 1-1) to the "●" (OFF) position to stop the device. The oxygen enriched air flow continues for approximately one minute after the device is stopped.

	Make sure during dissipation that the cannula is facing away from soft surfaces and clothing. Excess oxygen can accumulate and cause ignition if exposed to a spark or open flame.
	After turning the unit off, the user must wait 3-5 minutes before turning it back on. System pressure must dissipate before the unit will properly restart.

## CLEANING AND MAINTENANCE

### Cleaning

*Cleaning and disinfecting your device:* Only the outside of the **device** is to be cleaned. After making sure the Power Switch (Fig 1-1) is in the "●" (OFF) position, use a soft, dry cloth or, if necessary, a damp sponge, to wipe the cabinet enclosure. Then thoroughly dry with wipes and an alcohol based solution. This should be done daily and for each new patient.


	Acetone, solvents or any other inflammable products must not be used. Do not use abrasive powders.
---	--

*Cleaning and replacing filters:* The removable cabinet air filter (Fig 2-7) must be cleaned in warm water and household detergent. Dry before reinstalling. The inlet / silencer filter (Fig 3-11) should be inspected at each patient visit and replaced if required. The final product filter (not pictured) should only be replaced by a technician if required (not common).

*Cleaning and replacing accessories:* Clean the humidifier according to manufacturer's instructions. If no instructions are provided, do the following: empty the water from the humidifier, rinse the flask and lid under running water. Regularly disinfect the humidifier by immersing the flask and lid in a disinfectant solution (we recommend using a solution of 1 part vinegar to 10 parts water). Rinse under running water and dry. Tubing and cannula should be used according to the manufacturer's instructions and replaced for each new patient.

### Maintenance

No special maintenance needs to be carried out by the patient. Your equipment supplier performs periodic maintenance operations to assure continued reliable service from the *device*.

	DO NOT disassemble due to danger of electrical shock. Refer servicing to qualified service personnel.
---	---

The expected service life of this device is 10 years with routine preventive maintenance.

*Preventive Maintenance:* Wash cabinet filter (see “Cleaning and replacing filters”) weekly or after approximately 100 hours of use and for each new patient. More frequent cleaning is recommended in dusty environments. Inspect inlet air filter (Fig 3-11) at each patient visit. Replace filter annually, or more often depending on environment. Check oxygen concentration every 15,000 hours or 3 years to verify the continuing OCSI function.

The manufacturer’s instructions for the preventive maintenance of the devices are defined in the service manual, (PN 2010-2329). Check with your service provider for any updates to recommended schedules. The work must be carried out by suitably trained technicians certified by the manufacturer. Use original spare parts only (see “Accessories and Spare Parts”). Upon request, the supplier can provide circuit diagrams, spare parts lists, technical details or any other information of use to qualified technical personnel for parts of the device which are designated as being the manufacturer’s responsibility or by the manufacturer as repairable.


## DISPOSAL

### Method for Waste Disposal

All waste from the device (Patient Circuit, Filters, Etc.) must be disposed of using methods appropriate to the civil authority of the location where disposed.

### Disposing of the Device

This device has been supplied by an environmentally aware manufacturer. A majority of the parts in the device are recyclable.

Follow local governing ordinances and recycling plans regarding disposal of the device or components normally used in operation. Any accessories not original to the device must be disposed of in accordance with the individual product markings for disposal. Furthermore, as part of the marking directive 93/42/EEC, the serial number of the device disposed of must be sent to Nidek Medical if the unit has the  marking.

## TROUBLESHOOTING

Observations	Possible Causes	Solutions
The I-O (ON/OFF) button is in the “I” (ON) position but the device does not operate.	Mains cable (Fig 2-9) is not correctly plugged into the wall outlet.	Check the cable connection.
The no voltage detection alarm test does not work. (See Alarms and Safety Features)	Capacitor is not charged Internal electrical fault.	Check the circuit breaker (Fig 1-5) on the front of the unit; Reset if necessary.  Plug unit in for 10 minutes and retest.  Contact your equipment supplier.
The I-O (ON/OFF) button is in the “I” (ON) position, the compressor is operating and there is a flow but the green light is not lighted.	Faulty indicator.	Contact your equipment supplier.
The I-O (ON/OFF) button is in the “I” (ON) position but there is no flow. The audible alarm sounds continuously.	Pneumatic connection broken or other pressure problem.	Stop the device by pressing the I-O (ON/OFF) button and contact your equipment supplier.
The I-O (ON/OFF) button is in the “I” (ON) position, the compressor is operating and there is a flow but the audible alarm sounds continuously.	Internal electrical fault.  Pneumatic circuit fault or low purity.	Stop the device by pressing the I-O (ON/OFF) button and contact your equipment supplier.
The compressor stops in mid-cycle, then starts again after a few minutes.	Compressor thermal safety device has been activated.  Dirty Filters.  Cooling fan(s) not operating.	Stop the device and wait for it to cool down.  Clean cabinet filter. Restart. If the device does not start, contact your equipment supplier.  Stop the device by pressing the I-O (ON/OFF) button and contact your equipment supplier.
The oxygen enriched air flow is interrupted at the nasal cannula outlet.	Tube disconnected or humidifier cap is not tight.	Check that tubing connections are secure and that the humidifier is sealed.
The flow at the nasal cannula outlet is irregular.	Cannula tubing is kinked or restricted.	Straighten the tubing; contact your equipment supplier if damaged.

## EMC INFORMATION

<b>Appendix A: EMC Information</b>			
<p><b>Important:</b> Failure to follow these guidelines listed may result in increased emissions and/or decreased immunity of the subject device.</p> <ul style="list-style-type: none"> <li>• Medical Electrical Equipment needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in this manual.</li> <li>• Portable and mobile RF communications equipment can affect Medical Electrical Equipment.</li> <li>• The use of Accessories, transducers, and cables other than those specified by the manufacturer, may result in increased Emissions or decreased immunity of the device.</li> <li>• The device should not be used adjacent to or stacked with other equipment and that adjacent or stacked use is necessary, the device should be observed to verify normal operation in the configuration in which it will be used.</li> <li>• Use on Nidek Replacement electrical parts.</li> </ul>			
<p><b>Guidance and Manufacturer's Declaration – Electromagnetic Emissions</b>  <b>This device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment.</b></p>			
<b>Emissions Test</b>	<b>Compliance</b>	<b>Electromagnetic Environment – Guidance</b>	
RF Emissions CISPR 11	Group 1	This device uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.	
RF Emissions CISPR 11	Class B	This device is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.	
Harmonic Emissions IEC 61000-3.2	Class B		
Voltage Fluctuations /Flicker Emissions	Complies		
<p><b>Guidance and Manufacturer's Declaration - Electromagnetic Immunity</b>  <b>This device is intended for use in the electromagnetic environment specified below. The customer or the user of the device should assure that it is used in such an environment</b></p>			
<b>Immunity Test</b>	<b>IEC 60601 Test Level</b>	<b>Compliance</b>	<b>Electromagnetic Environment - Guidance</b>
Electrostatic Discharge (ESD) IEC 61000-4-2	± 6kV contact ± 8kV Air	Complies	Floors should be wood, concrete, or ceramic tile. floors are covered with synthetic material, the relative humidity should be at least 30%.
Conducted RFI IEC 61000-4-6	3 Vrms 150 kHz to 80 Hz	Complies	Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey should be less than the compliance level ( 3 V/m ) in each frequency range. Interference may occur in the vicinity of equipment marked with the following symbol: Portable and mobile RF communications equipment should be used no closer to any part of the device, including cables, than the distance calculated from the equation applicable to the frequency of the transmitter. $d = 1.2 \sqrt{P}$ (80-800MHz) $P$ =Transmitter power level in watts $d = 2.3 \sqrt{P}$ (800MHz-2.5GHz) $d$ =distance in meters
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.5 GHz	Complies	
Electrical fast transient/burst IEC 61000-4-4	± 2 kV for power supply lines ± 1 kV for input/output lines	Complies	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	± 2 kV for power supply lines ± 1 kV for input/output lines	Complies	Mains power quality should be that of a typical commercial or hospital environment.
Power frequency (50/60Hz) Magnetic field IEC 61000-4-8	3 A/m	Complies	Power frequency magnetic fields should be at levels characteristic of the typical location in a typical commercial or hospital environment
Voltage Dips, short interruptions and voltage variations on power supply input line. IEC 61000-4-8	<5% $U_T$ (>95% dip in $U_T$ ) for 0.5 cycles	Complies	Mains power quality should be that of a typical commercial or hospital environment. If the user of this device requires continuous operation during power mains interruption, it is recommended that the device be powered from an uninterruptible power supply (UPS).
	40% $U_T$ (60% dip in $U_T$ ) for 5 cycles	Complies	
	70% $U_T$ (30% dip in $U_T$ ) for 25 cycles	Complies	
	<b>Note:</b> $U_T$ is the a.c. mains voltage prior to the application of the test levels	<5% $U_T$ (>95% dip in $U_T$ ) for 5 seconds	

## CONFORMITY WITH EN 60601-1



### CONFORMITY WITH EN 60601-1 (§ 6.8.2 b):

The manufacturer, assembler, installer or distributor are not considered to be responsible themselves for the consequences on the safety, reliability and characteristics of a device unless the:

- Assembly, fitting, extensions, adjustments, modifications or repairs have been performed by persons authorized by the party in question.
- Electrical installation of the corresponding premises complies with local electrical codes. (e.g. IEC/NEC)
- Device is used in accordance with the instructions for use.

If the replacement parts used for the periodic servicing by an approved technician do not comply with the manufacturer's specifications, the manufacturer is not responsible in the event of an accident or non-performance. This device complies with the requirements of the FDA Quality System Regulation and 93/42/EEC European directive but its operation may be affected by other devices being used nearby, such as diathermy and high frequency electrosurgical equipment, mobile telephones, CB and other portable devices, microwave ovens, induction plates or even remote control toys or any other electromagnetic interferences which exceed the levels specified by the EN 60601-1-2 standard.

# NIDEK

*Medical*

**Nidek Medical Products, Inc.**  
3949 Valley East Industrial Drive  
Birmingham, Alabama 35217 U.S.A.  
Tel: 205-856-7200 Fax: 205-856-0533

**EU Representative**  
mdi Europa GmbH  
Langenhagener Str. 71  
30855 Hannover-Langenhagen  
Germany  
Tel: +49-511-39-08 95 30  
Fax: +49-511-39-08 95 39  
info@mdi-europa.com  
www.mdi-europa.com